





freePEMF duo quadro-rotating field mat

Chair – view from the top

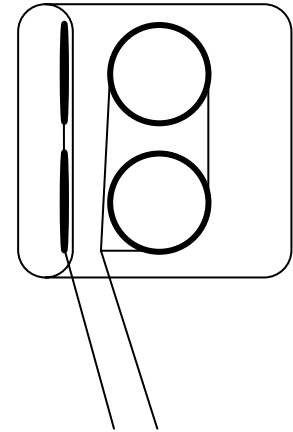

50 turns (coils) coil. Use fi 0.4mm diameter Cu wire.

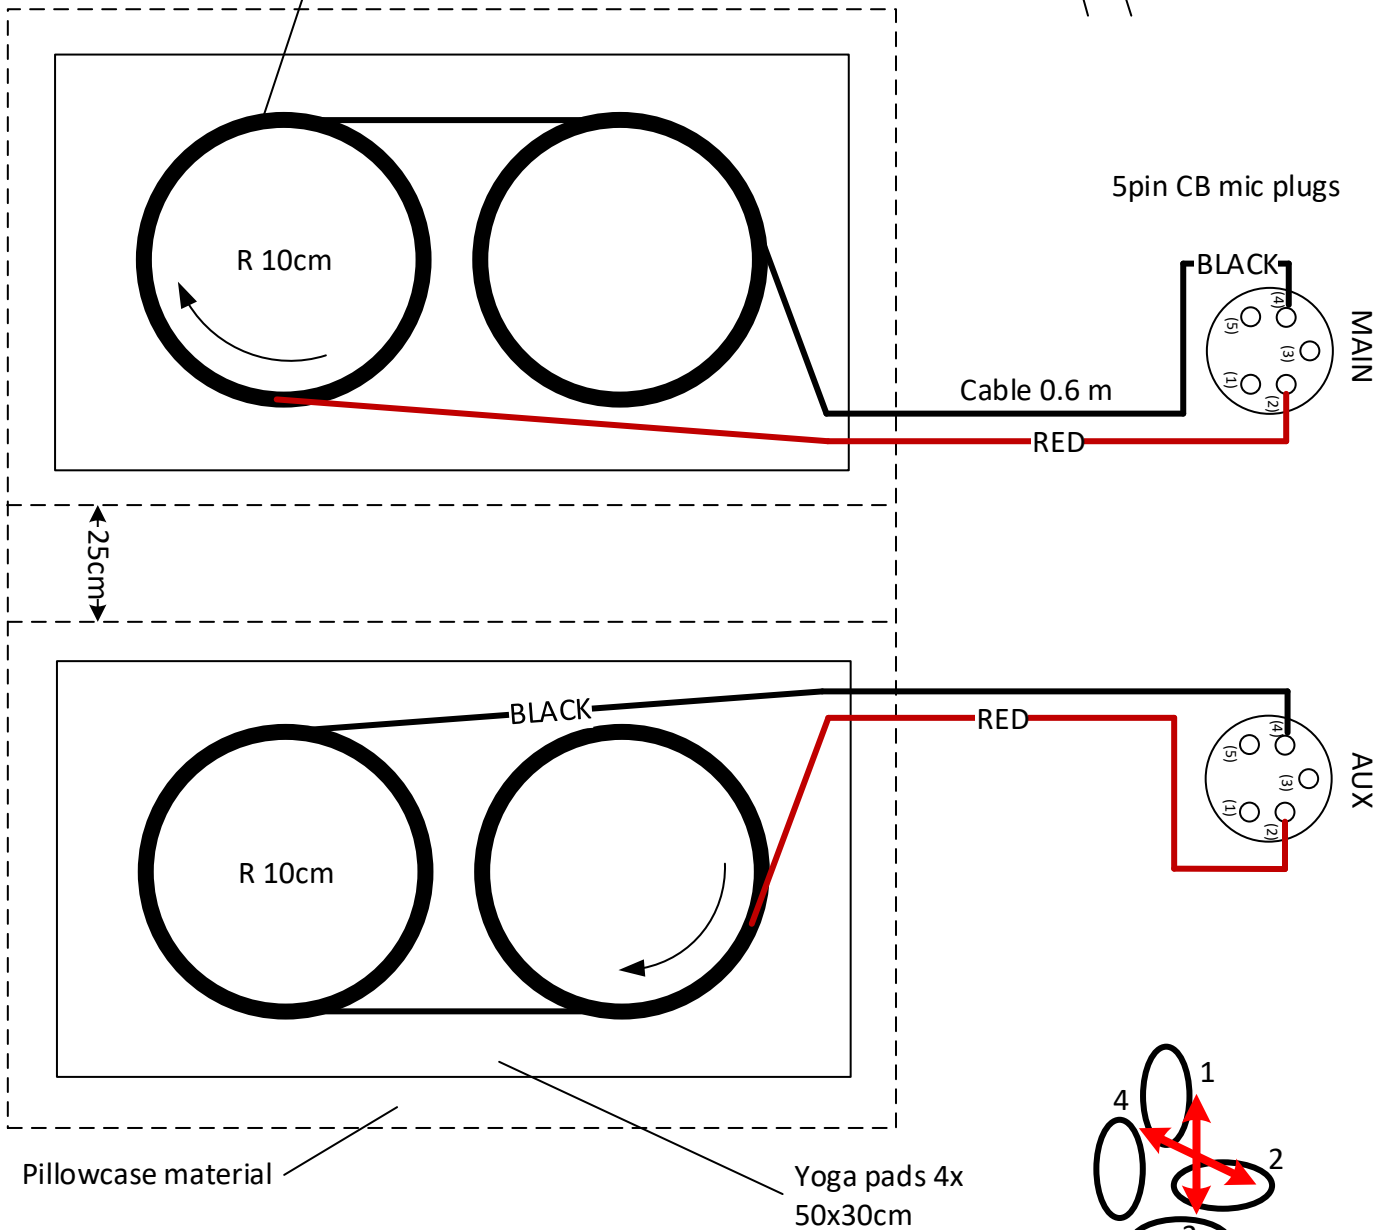

Coil assembly: <https://biotronika.pl/en/coil-assembly>

freePEMF duo assembly: <https://biotronika.pl/en/diy-freePEMF-duo>

Therapies: <https://biotronika.pl/en/terapie>